



1/9

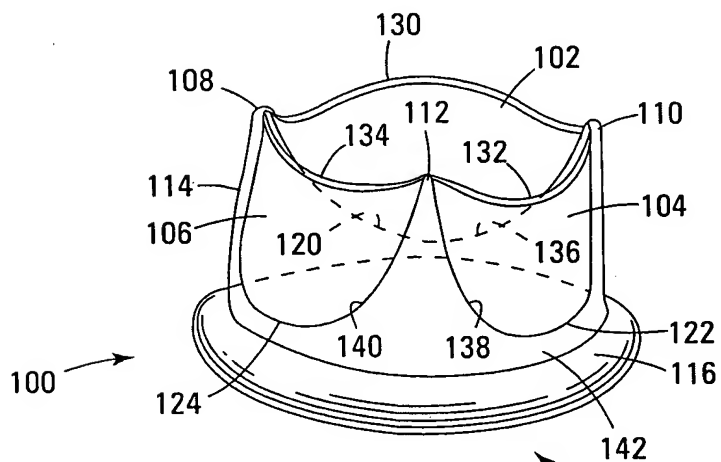


Fig. 1

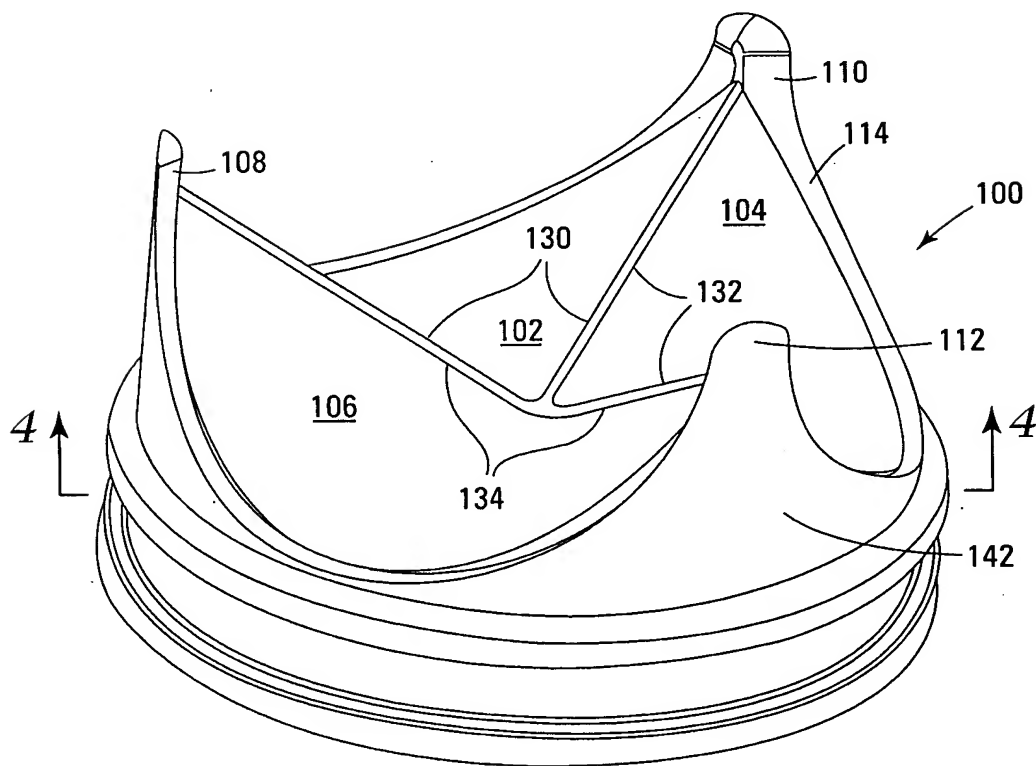


Fig. 2



2/9

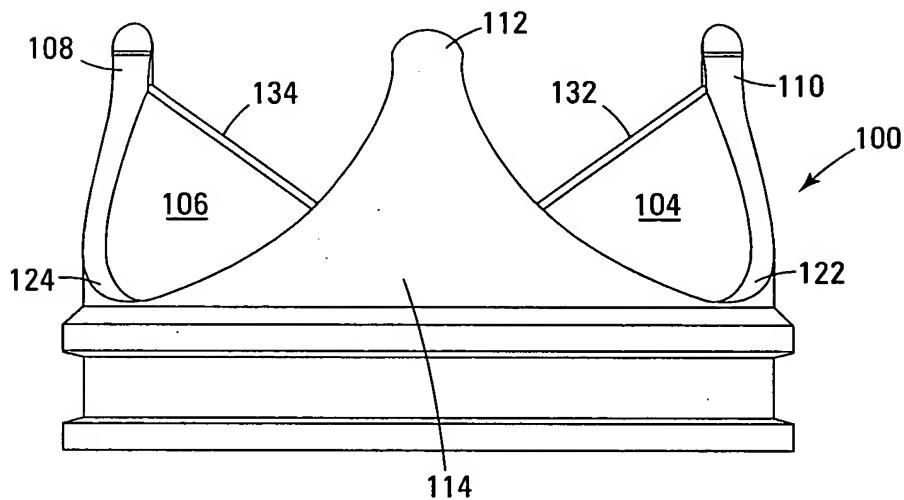


Fig. 3

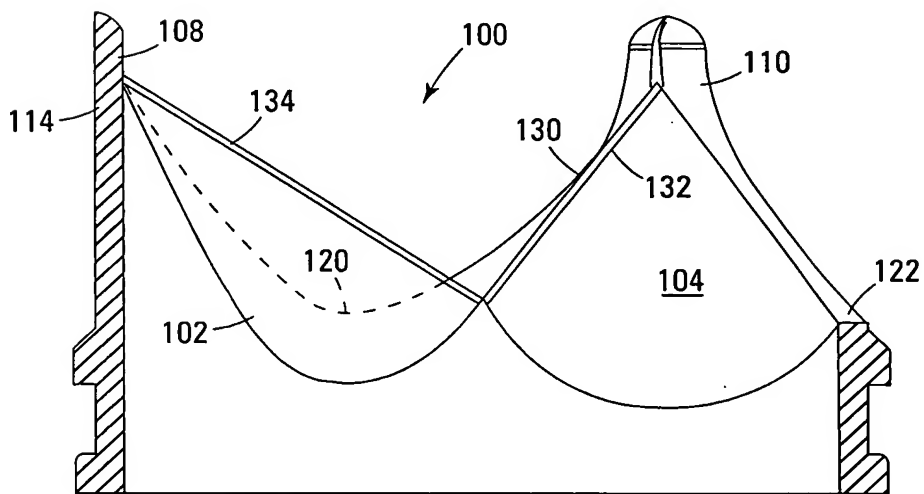


Fig. 4

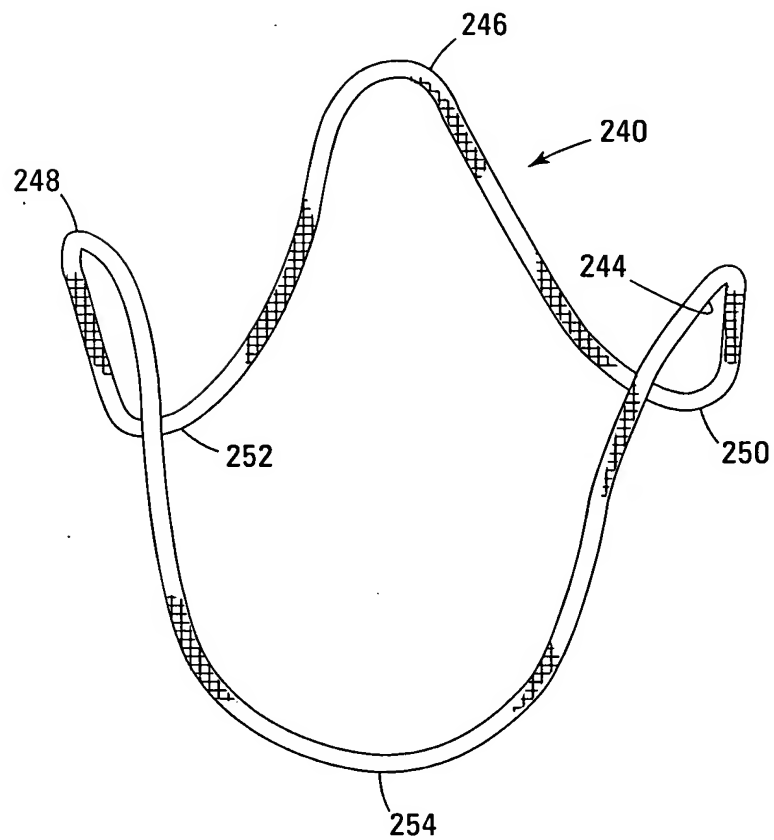


Fig. 5



4/9

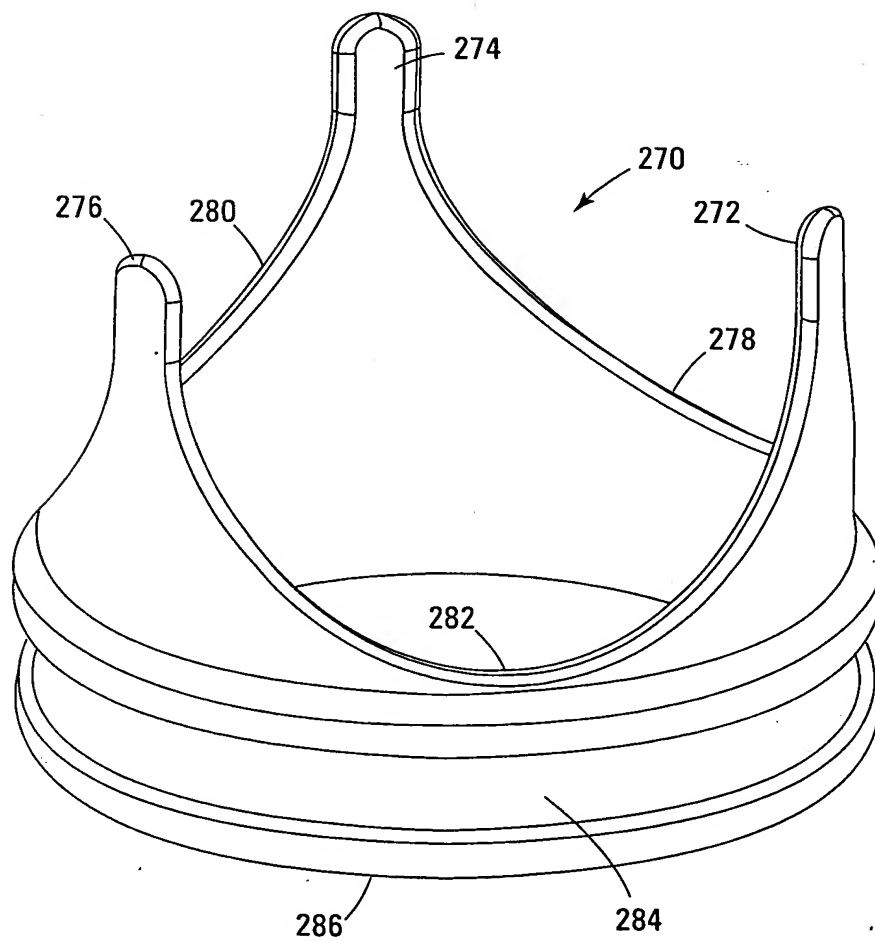


Fig. 6

OCT 14 2003
PATENT & TRADEMARK OFFICE

5/9

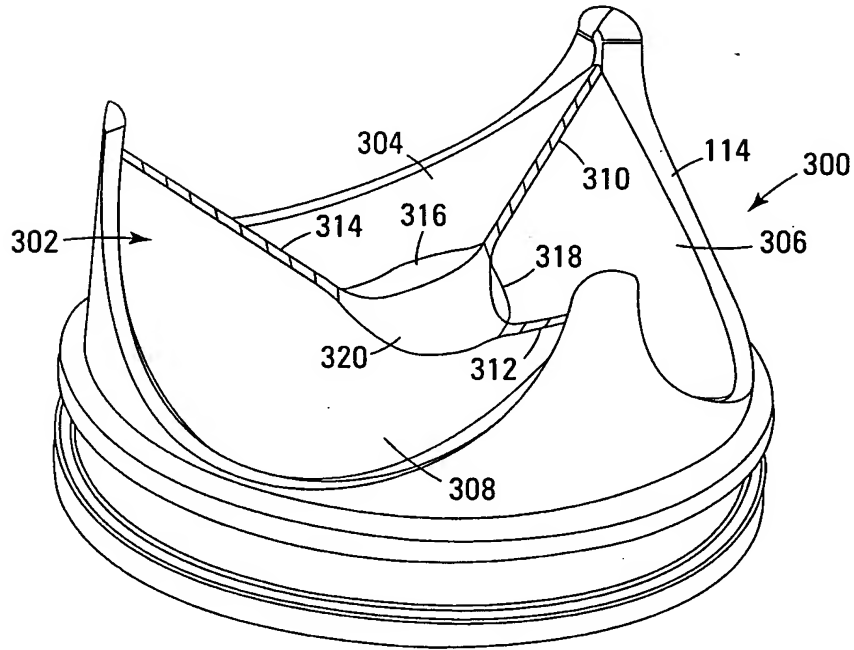


Fig. 7

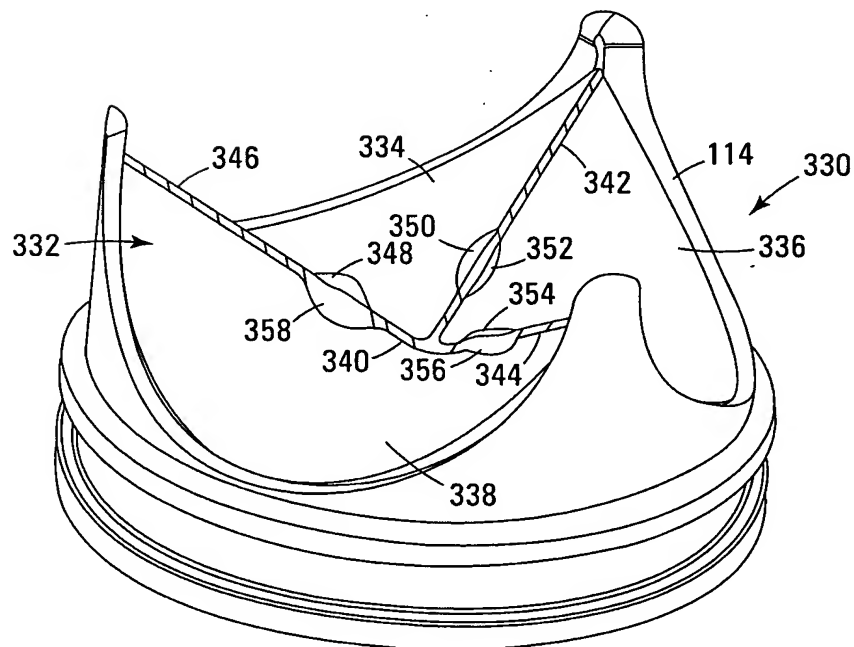


Fig. 8



6/9

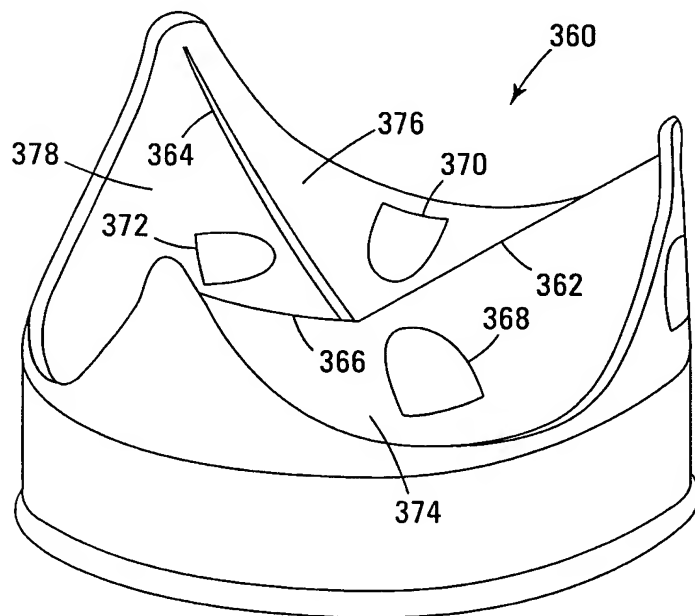


Fig. 9

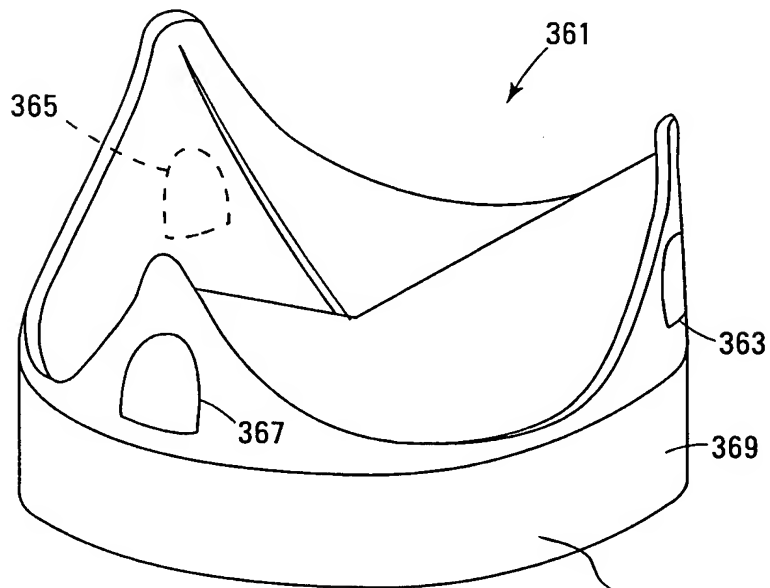


Fig. 10



Applicant: Kruse, et al.
Title: FATIGUE TEST FOR PROSTHETIC STENT
Atty Docket No. 01610.0108-US-01 Serial No. 10/034,694

7/9

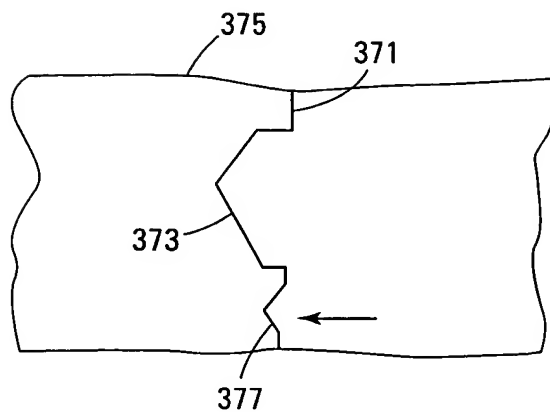


Fig. 11



8/9

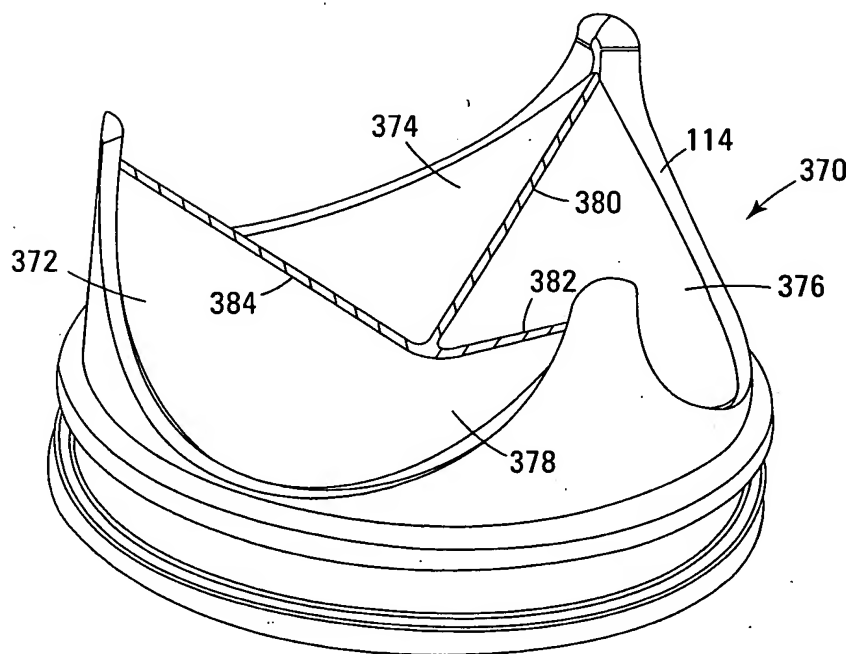


Fig. 12

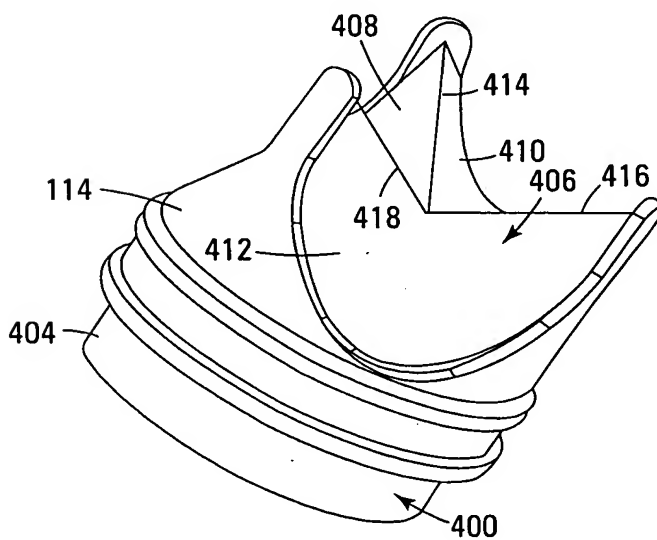


Fig. 13



9/9

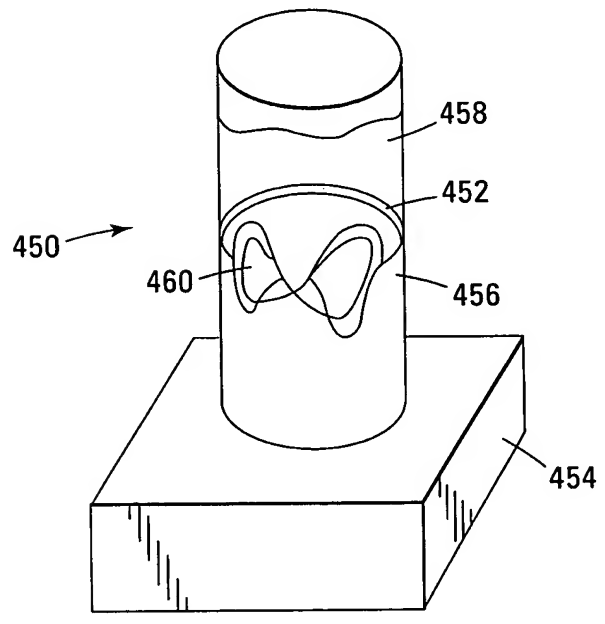


Fig. 14

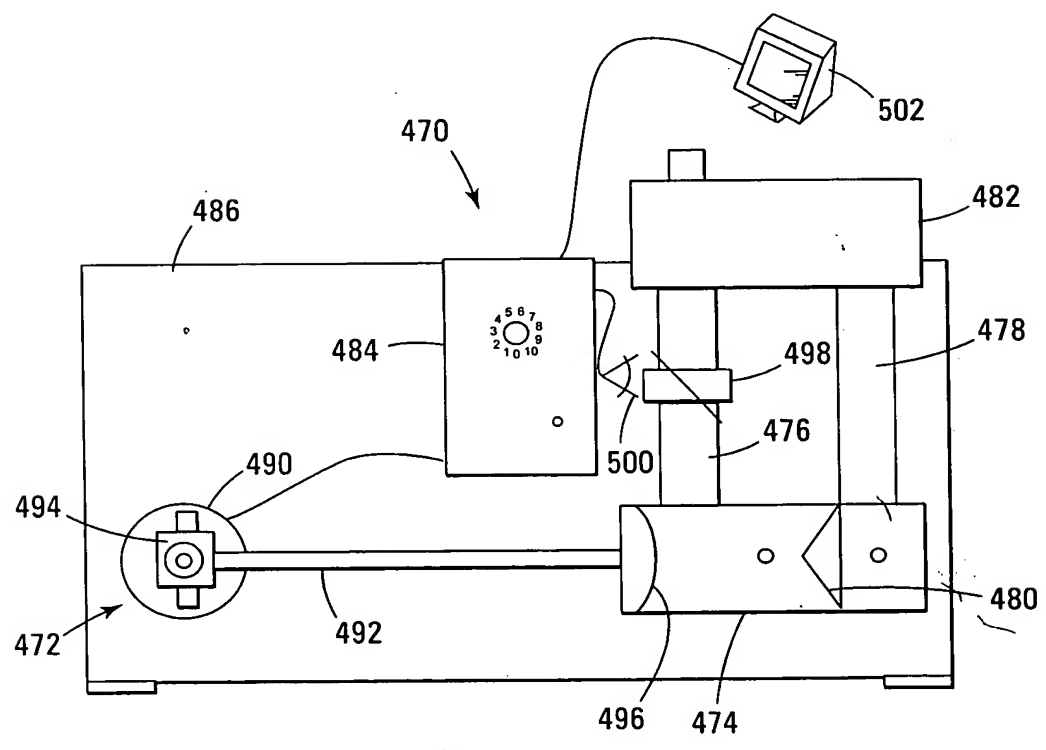


Fig. 15